



## Performance of a scintillating fibres semiprojective electromagnetic calorimeter

M. Bertino, C. Bini, G. De Zorzi, G. Diambri Palazzi, G. Di Cosimo, A. Di Domenico, F. Garufi, P. Gauzzi and D. Zanello

Dipartimento di Fisica, Universita' "La Sapienza", Roma,  
and INFN Sezione di Roma, P.le A.Moro 2,00185 Roma, Italy

A highly segmented scintillating fibres / lead electromagnetic calorimeter has been tested. Each calorimeter module has semiprojective geometry and is shaped as a wedge with an angle of  $(0.82)^\circ$ . The fibres are however parallel to the wedge axis and the two small lateral regions are not fibre-instrumented. This simple and cheap approach to a projective geometry allows to achieve still good energy and space resolution. Results with electrons in the range 10-100 GeV are presented.

### 1. INTRODUCTION

We have studied a lead-scintillating fibres segmented electromagnetic calorimeter with a semiprojective geometry. The modules have the shape of a truncated pyramid, in such a way that the sides are pointing towards an axis at a distance of 1.43 m. Figure 1a shows the geometry of a module.

The main feature of this calorimeter is that the fibres fill only the parallelepiped part of a module, so that the two small lateral regions are not fibre-instrumented. The purpose of our test has been to verify how much the calorimeter performance, in terms of energy and space resolution, is affected by the loss of energy deposited in the wedge-shaped regions, which are not sampled.

The calorimeter is segmented in 25 modules, 35 cm long, of  $20.5 \times 20.5 \text{ mm}^2$  (front) and  $25.5 \times 20.5 \text{ mm}^2$  (back) cross area. The main features of the calorimeter are summarized in table 1.

### 2. TEST AND RESULTS

The test was performed at the CERN-SPS. The calorimeter was placed on a platform movable with respect to the electron beam both in the horizontal and vertical directions. A telescope of two delay wire chambers in front of the calorimeter was used to measure the electron impact point, with a space accuracy of about 0.2 mm. The calorimeter was operated with a tilt angle of  $2.5^\circ$  in both horizontal and vertical directions.

#### 2.1 Energy response and resolution

Figure 1b shows the detected energy as a function of the electron impact position for three calorimeter modules along horizontal and vertical directions, at an electron energy of 50 GeV. In the x-coordinate there is a systematic difference of about 20% between the measurement of the energy at the centre and at

Table 1  
Main calorimeter features

Scintillating fibres	Kuraray SCSF81, 1 mm diameter
Absorber alloy (% in weight)	AF17 (52.5% Bi, 32% Pb, 15.5% Sn)
Volume ratio fibres : absorber	1 : 3.17
Average density	$7.1 \text{ g/cm}^3$
Average radiation length	1.0 cm
Average Moliere radius	2.3 cm
Module cross area	$20.5 \times 20.5 \text{ mm}^2$ (front)
(horizontal x vertical)	$25.5 \times 20.5 \text{ mm}^2$ (back)
Calorimeter total cross area	$10 \times 10 \text{ cm}^2$ (front)
Calorimeter total length	35 cm

the border of the modules, but as the impact point is measured by the calorimeter itself a correction can be applied to the detected energy. The two dips correspond to the two non-instrumented wedge-shaped regions.

The calorimeter response turns out to be linear within 2% in the explored energy range 10-100 GeV, as shown in fig. 2a. The linearity does not depend on the electron impact position on the module.

The energy resolution  $\sigma/E$  is a linear function of  $1/\sqrt{E(\text{GeV})}$  as shown in fig.2b, but there is some dependence on the impact position (see fig.1b) :

$$\sigma/E = (13.9 \pm 0.9)\%/\sqrt{E(\text{GeV})} + (1.4 \pm 0.2)\%, \text{ at the module centre;}$$

$$\sigma/E = (11.0 \pm 1.0)\%/\sqrt{E(\text{GeV})} + (0.6 \pm 0.4)\%, \text{ at the middle of the module x-border;}$$

$$\sigma/E = (14.0 \pm 1.0)\%/\sqrt{E(\text{GeV})} + (2.0 \pm 0.5)\%, \text{ at the middle of the module y-border.}$$

The x-border corresponds to an electron impinging between two modules, where only a fraction of the e.m. shower energy is sampled because the fibres are missing in the wedge-shaped volume.

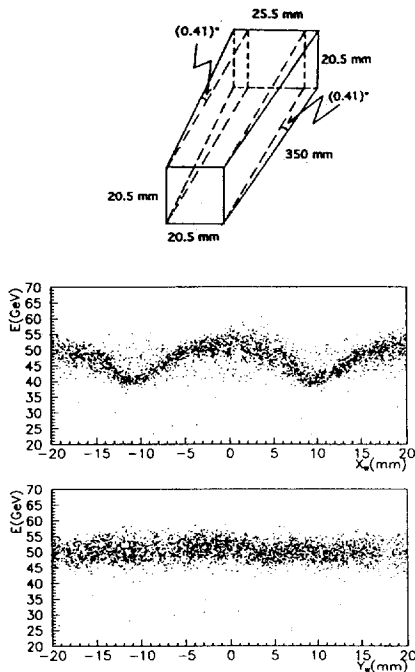


Fig. 1: a) Schematic view of a semiprojective module. b) The calorimeter response uniformity in the horizontal and vertical directions for 50 GeV electrons

The y-border corresponds to the separation between two modules with full energy sampling.

The energy resolution of this calorimeter is in agreement with the typical performance of a 'spaghetti calorimeter' [1,2]. The present result is also comparable to the performance of the semiprojective [3] and fully projective [4] 'spaghetti' calorimeters having full fibre instrumented modules.

Moreover it should be noticed that the energy resolution turns out to be slightly better near the non-instrumented region (i.e. at the x-border) respect to the whole detector. Although the signal in this region is reduced by 20% with respect to the central region (see fig. 1b), the signal fluctuation is reduced even more. We do not have a simple explanation for this phenomenon.

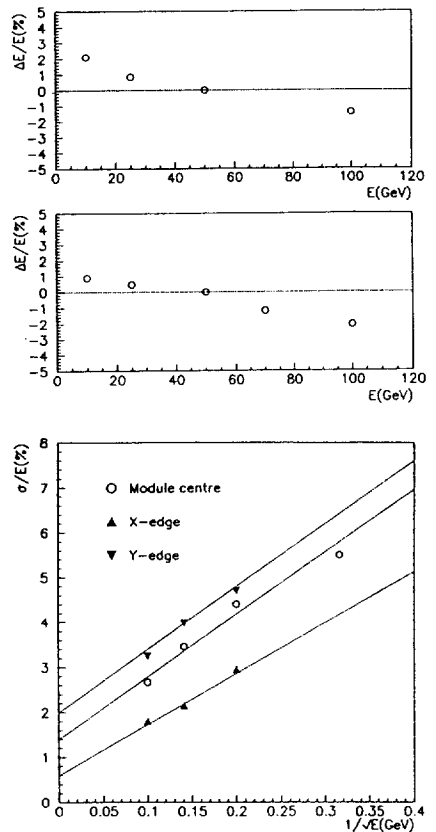


Fig. 2: a) Percentage non-linearity versus energy for a vertical tilt angle of  $2.5^\circ$  (up) and  $5^\circ$  (down). b) Energy resolution as a function of  $1/\sqrt{E(\text{GeV})}$  for the beam hitting the module centre (circles), the x-border (upward triangles), and the y-border (downward triangles). The vertical tilt angle is  $2.5^\circ$ .

### 2.2 Impact point resolution

Horizontal and vertical scans of the beam were done, in order to explore the space reconstruction accuracy of the calorimeter, along the x-coordinate and the y-coordinate, for the three central modules. The electron energy was 25, 50, and 100 GeV.

The (x,y) position is directly measured by the calorimeter by the energy deposited in the modules surrounding the e.m. shower vertex. This can be done by a simple 'centre of gravity' algorithm but, as usual for segmented detectors, a better impact point determination can be achieved by more sophisticated algorithms.

We have parametrized the dependence of the 'centre of gravity' coordinate on the 'true' coordinate with the following formula [5] :

$$x_g = a + b \arctan [ c ( x_w + d ) ] \quad (1)$$

where :  $x_w$  is the  $x$ -coordinate measured with the chambers;  $x_g$  is the  $x$ -coordinate measured with the calorimeter utilizing the simple 'centre of gravity' algorithm; a, b, c, and d are four parameters which are determined by fitting the experimental points ( $x_w, x_g$ ) with the function (1). The same formula holds for the y-coordinate. Figure 3a shows the  $x_g$  coordinate versus the  $x_w$  coordinate for 50 GeV electrons detected in the three central modules: the waving behaviour is typical of any modular calorimeter.

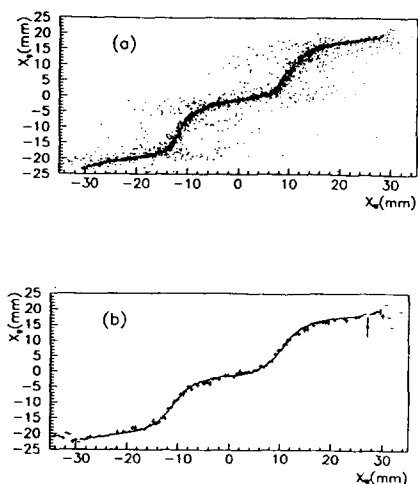


Fig. 3: a)  $x$ -coordinate measured by the beam chambers versus the coordinate reconstructed by the calorimeter with a simple 'centre of gravity' algorithm for 50 GeV electrons. b) The same result is shown with superimposed the fit of equation (1).

Figure 3b shows the  $x$ -coordinate data with the fit of equation (1) superimposed. The fit is carried on from a module centre to the adjacent module centre. The values of the four fitted parameters do not depend on the electron energy in our energy interval.

The parametrization (1) can be inverted as follows:

$$x_c = - d + ( 1/c ) \tan [ ( x_g - a ) / b ] \quad (2)$$

and applied event by event in order to obtain an unbiased  $x_c$  coordinate from  $x_g$ .

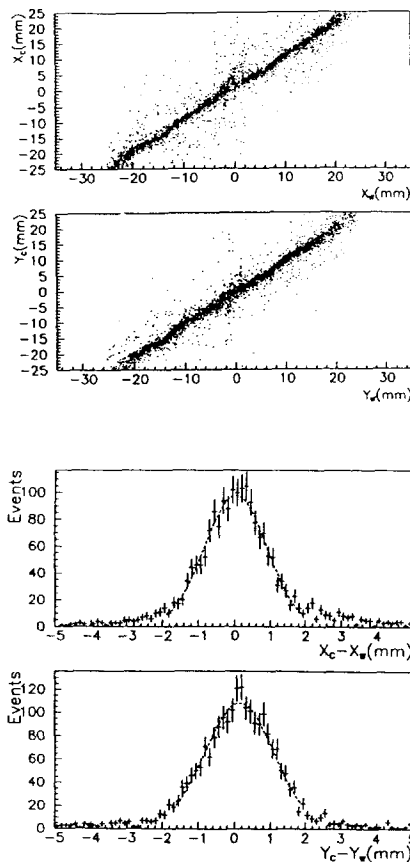


Fig. 4: (a)  $x$ - coordinate determined by the calorimeter with the algorithm of equation (2) versus the  $x$ -coordinate measured by the beam chambers. The centre of a module is at -20, 0, and 20 cm respectively. b) Same plot for the y-coordinate. c) Distribution of the difference between the calorimeter reconstructed abscissa (see equation (2)) and the 'true' one at 50 GeV. Fitting a gaussian function one finds  $\sigma_x = 0.87$  mm. d) Same plot for the y-coordinate; the gaussian fit gives  $\sigma_y = 0.94$  mm.

The waving behaviour in both horizontal and vertical coordinates is clearly reduced to an almost straight line by applying the equation (2). Figure 4a shows  $x_C$  ( $y_C$ ) versus  $x_W$  ( $y_W$ ) at 50 GeV. A small residual waving is still present, but it does not deteriorates the space resolution which is basically determined by the width of the ( $x_W$ ,  $x_C$ ) distribution, and ( $y_W$ ,  $y_C$ ) distribution, for the horizontal and the vertical coordinate respectively.

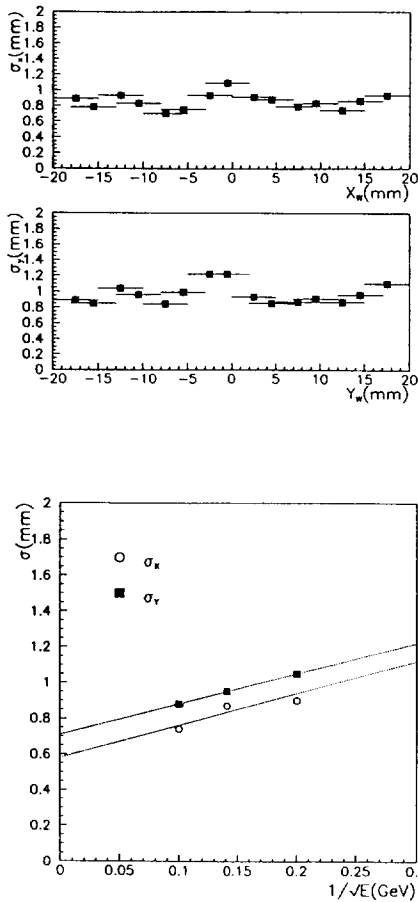


Fig. 5: a) Impact position resolution in  $x$ -coordinate and in  $y$ -coordinate, as a function of the impact position  $x$  and  $y$  respectively. The module centre is at about 0 cm, and its edges at -10 cm and 10 cm. The electron energy is 50 GeV. b) Impact point resolution of the electron shower as a function of the electron energy for the horizontal (circles) and the vertical (squares) coordinate respectively. The linear fit in  $1/\sqrt{E(\text{GeV})}$  gives the result quoted in section 2.

An example of impact points distribution as a function of the difference ( $x_W - x_C$ ) and ( $y_W - y_C$ ), is given in the fig. 4b at 50 GeV. The impact point resolution turns out to be slightly dependent on the impact position, as shown in fig. 5a at 50 GeV for both coordinates.

After all corrections the space resolution is a linear function of  $1/\sqrt{E(\text{GeV})}$

$$\sigma_x = (1.8 \pm 0.1) \text{ mm } / \sqrt{E(\text{GeV})} + (0.6 \pm 0.1) \text{ mm}$$

$$\sigma_y = (1.7 \pm 0.1) \text{ mm } / \sqrt{E(\text{GeV})} + (0.7 \pm 0.1) \text{ mm}.$$

This result is obtained by averaging  $\sigma$  over the full module size and is plotted in fig. 5b.

It is worth noting that the resolution is the same in both  $x$  and  $y$  coordinates. The different energy sampling at the two module borders in the horizontal coordinate does not affect the impact point reconstruction accuracy of this calorimeter.

The present result should be compared with the resolution obtained with highly segmented [2] and less segmented calorimeters [1,6], and furthermore having different fibre : lead volume ratio.

### 3. CONCLUSIONS

A simple approach to the design of a segmented semiprojective e. m. calorimeter has been carried out. The main feature of this calorimeter is that the wedge-shaped lateral region, at both the sides of a module, is not filled with fibres.

The energy and the space resolution have been measured on an electron beam in an energy range from 10 to 100 GeV.

Our results show that both these features are uniform over the whole calorimeter, i.e. no worsening effect is found when the electron hits the wedge-shaped regions. The energy resolution compares with the common values of the so called spaghetti calorimeters:  $\sigma/E = 14.0\% / \sqrt{E(\text{GeV})} + 1.5\%$ . The space resolution, in both the coordinates, is as good as that obtained with highly segmented, but non-projective, fibres/lead calorimeters:  $\sigma = 1.7 \text{ mm } / \sqrt{E(\text{GeV})} + 0.6 \text{ mm}$ .

## REFERENCES

1. R. Wigmans, Nucl. Instr. and Meth. A 315 (1992) 299.
2. A. Asmone et al., Nucl. Instr. and Meth. A 326 (1993) 477.
3. B. Bencheikh et al., Nucl. Instr. and Meth. A 315 (1992) 354.
4. J. Badier et al., CERN-PPE/93-20 (1993).
5. D. Acosta et al., Nucl. Instr. and Meth. A 305 (1991) 55.
6. S. Dagoret et al., CERN-PPE/93-147 (1993).